

● 本院是政府计量行政管理部门依法设立的法定计量检定机构

This laboratory is a legal metrological verification institution established by the government metrological administrative department according to the law.

● 本院质量管理体系符合ISO/IEC17025标准的要求。

The quality management system for laboratory complies with ISO/IEC 17025 standards.

● 本次校准的技术依据(名称、代号)

Reference documents for the Calibration (Name, Code)

依据: JJG 1004-2012 电磁感应分压器

依据: JJG 1004-2012 数字高压表校准规范

依据: JJG 1004-2012 数字多用表校准规范

● 本次校准使用的主要计量标准器具

Main measuring standards used in this calibration

名称/名称

型号/Model

证书编号/Cert. No.

名称/名称

型号/Model

证书编号/Cert. No.

感应分压器

FG2/7216

第20221173号

数字高压表

ERC-150M211090603

2022DW023300217/2023-01-02

数字多用表

34401A/MY45016530

2022DW02310639/2023-06-19

● 校准环境条件

Environmental condition on the Calibration

温度: 16.6℃

相对湿度: 46 %

其它: _____

Temperature

R.H.

Others

气压: _____

地点: 现场

原始记录编号: _____

Pressure

Place

Record No.

本校准结论, 仅对受校样品的本次校准有效。

It's Effect That Results of This Report Relate Only To The Sample(s) Calibrated.






2024.11



2024.11.28

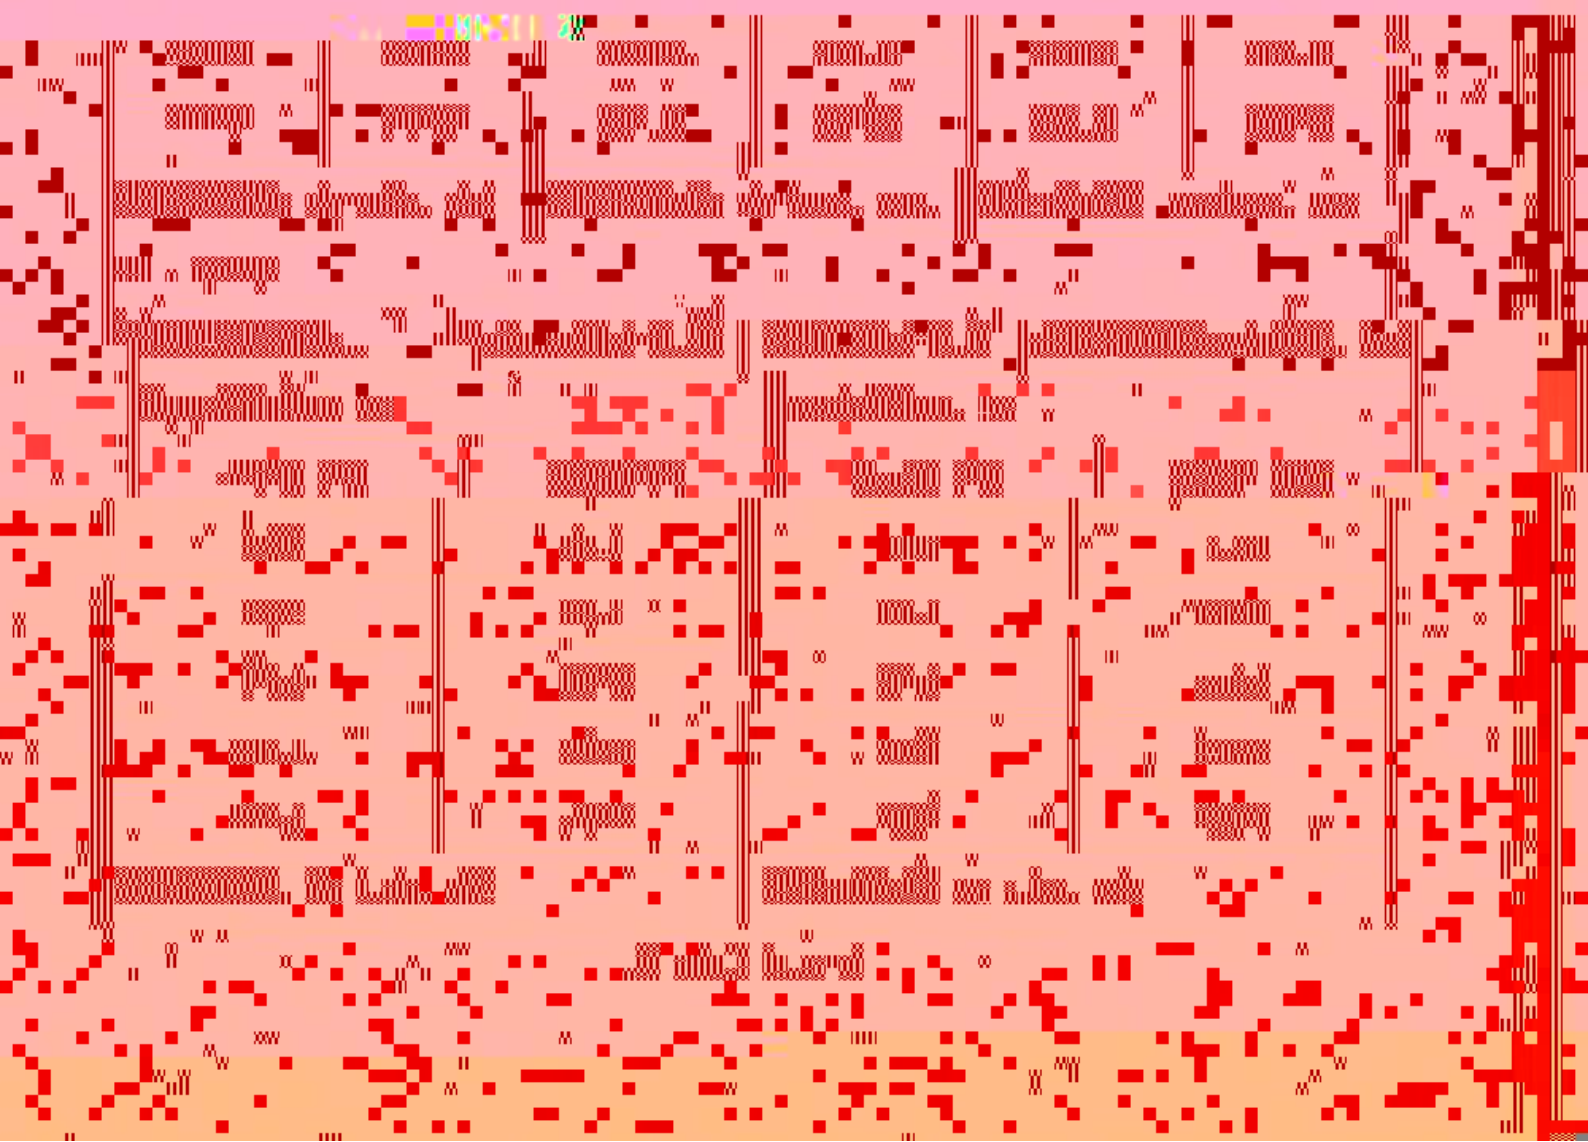

校准证书

标准变比值	实测变比值	测量不确定度 U , $k=2$
5	4.9998	± 0.0060
10	10.001	0.009
30	30.008	0.030
50	50.004	0.050
100	100.00	± 0.15

三

新到

11